



Replacement Sheets

1/9

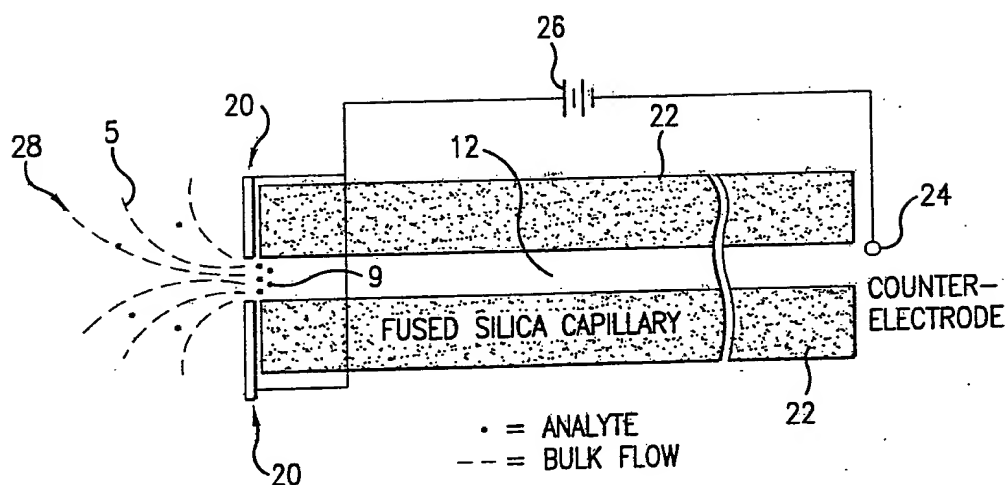


FIG.1



Replacement Sheets

2/9


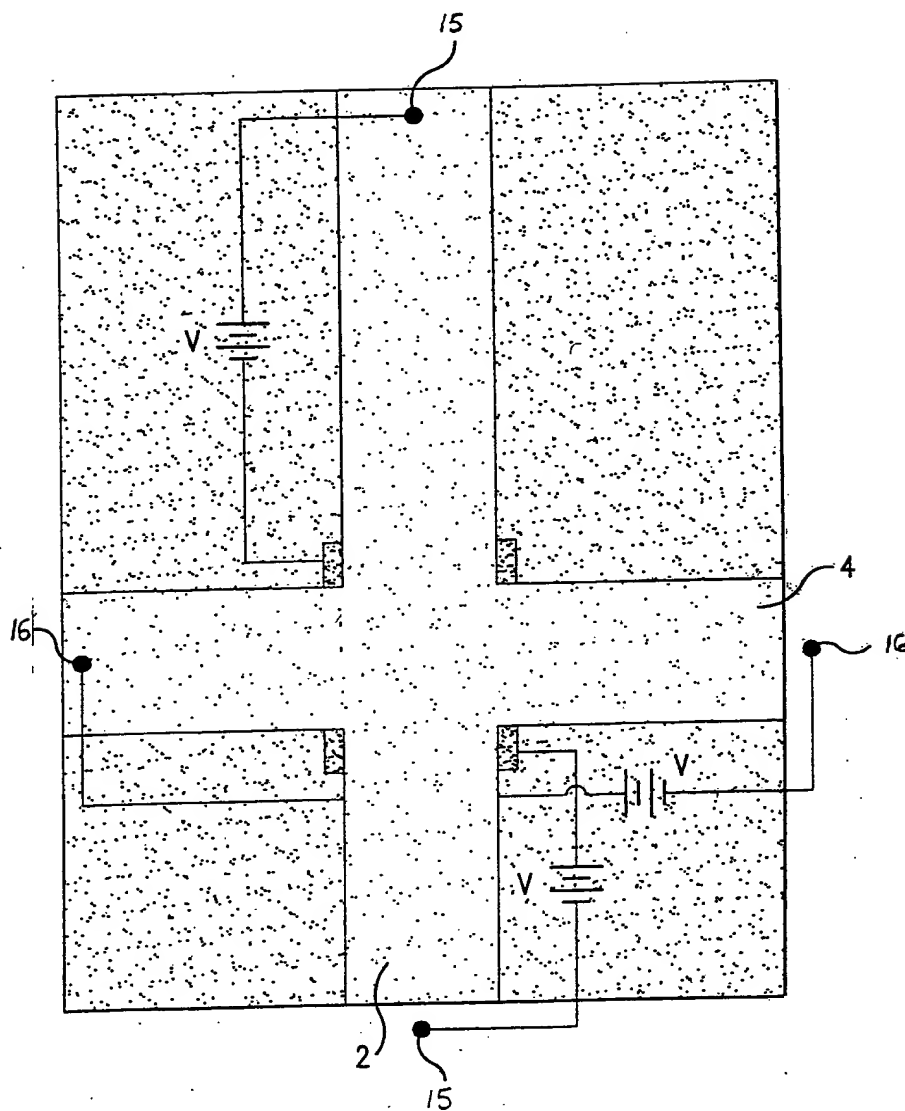


FIG.2a



Replacement Sheets

3/9

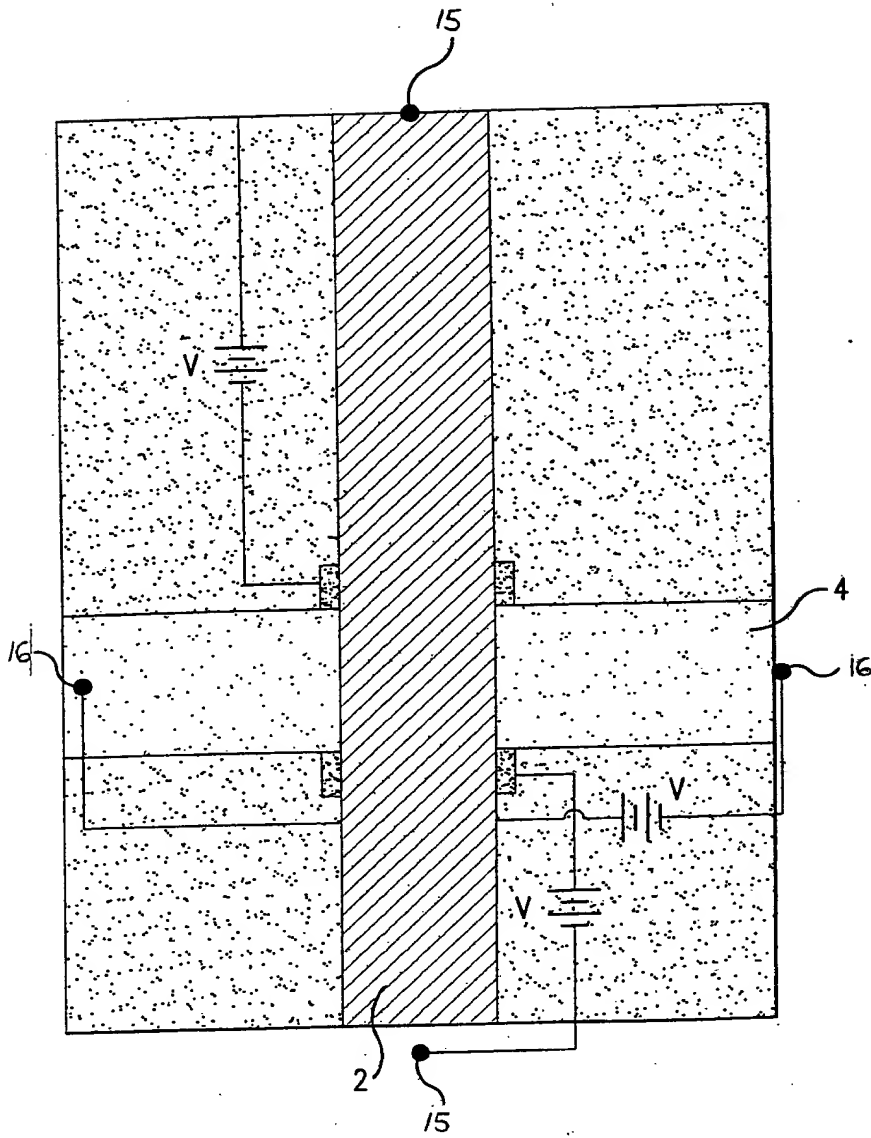


FIG.2b



Replacement Sheets

4/9


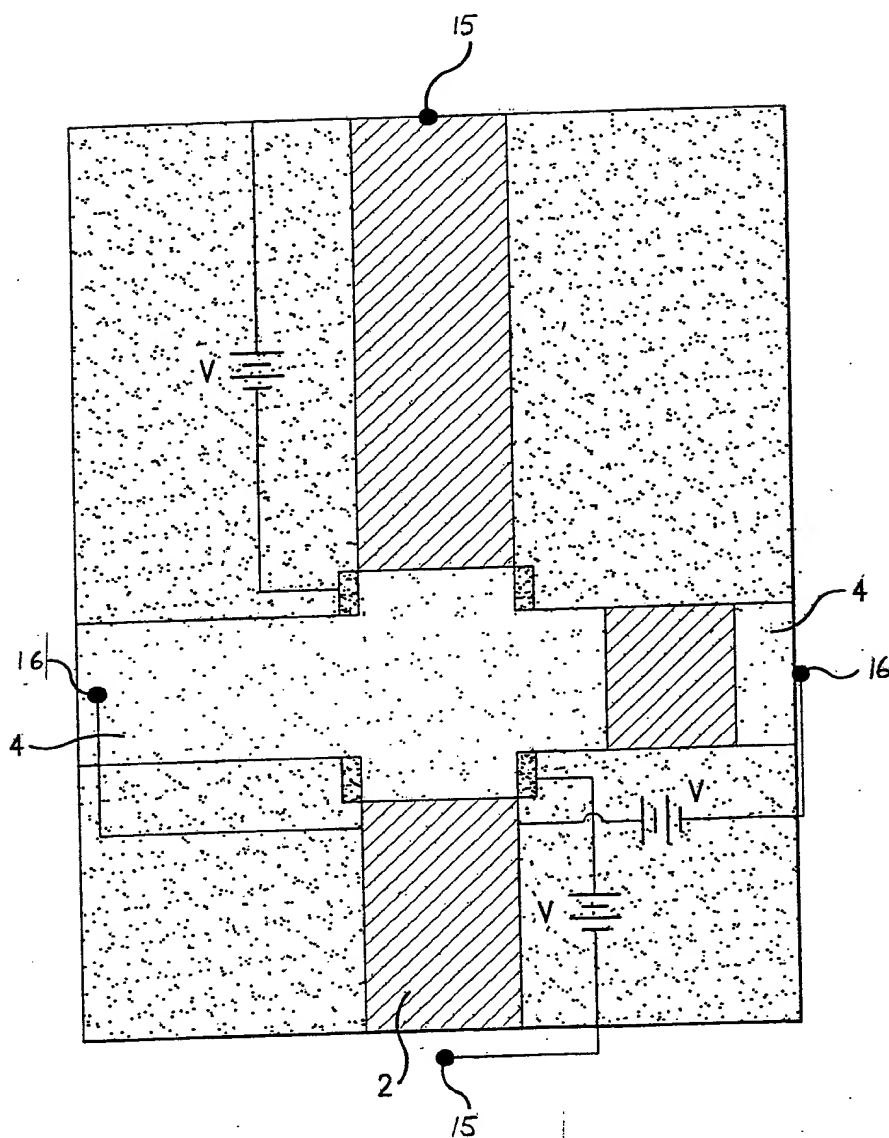


FIG.2c



Replacement Sheets

5/9

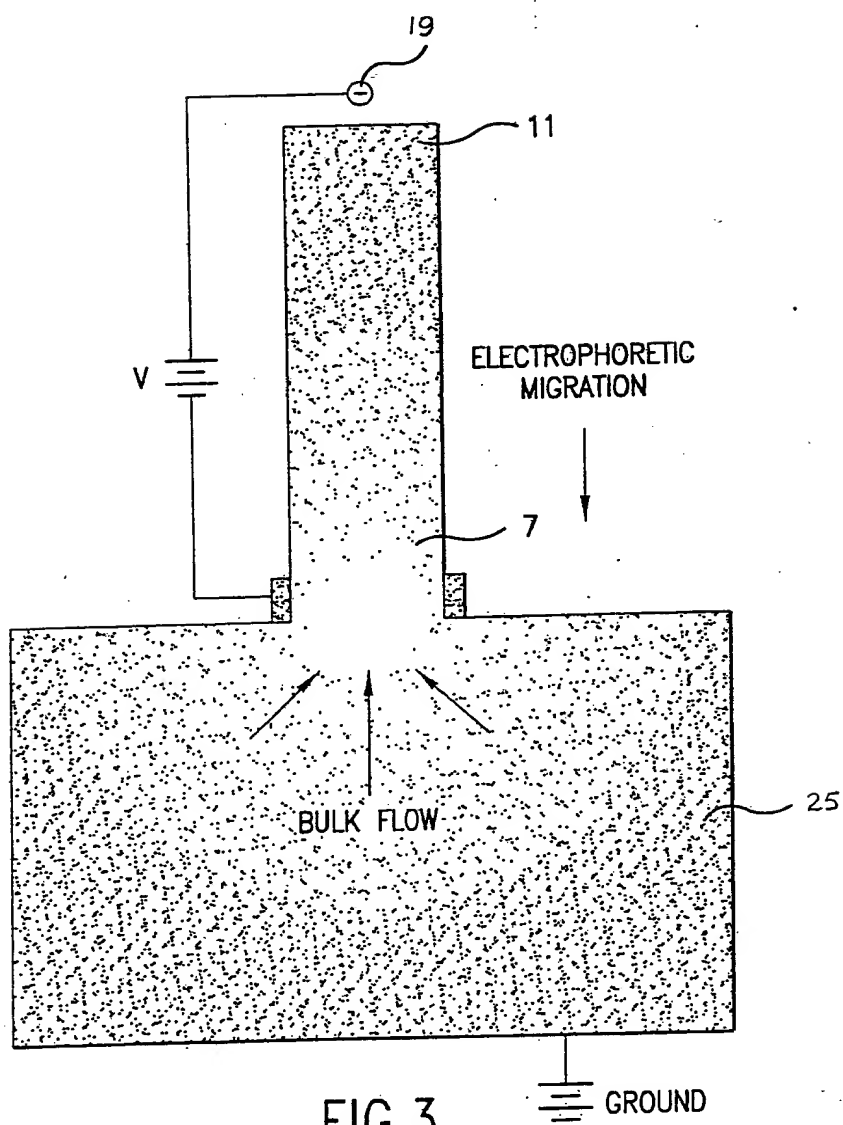



FIG.3


GROUND



Replacement Sheets

6/9

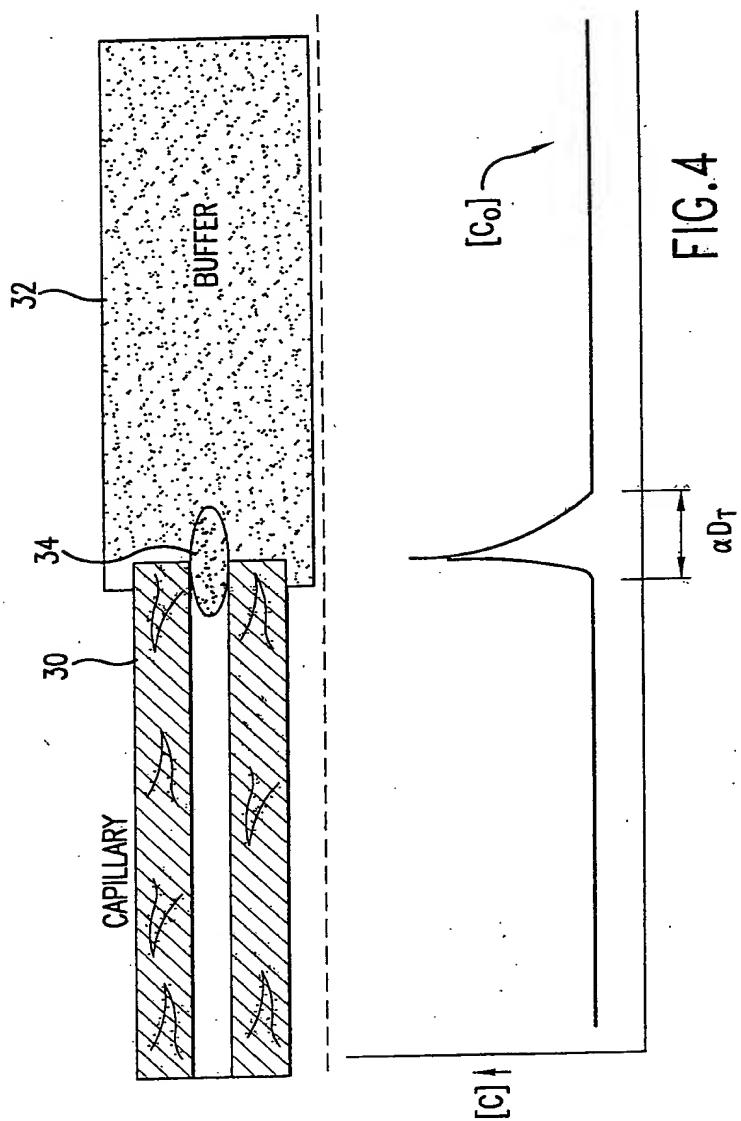




Replacement Sheets

7/9


FLUORESCENCE INTENSITY

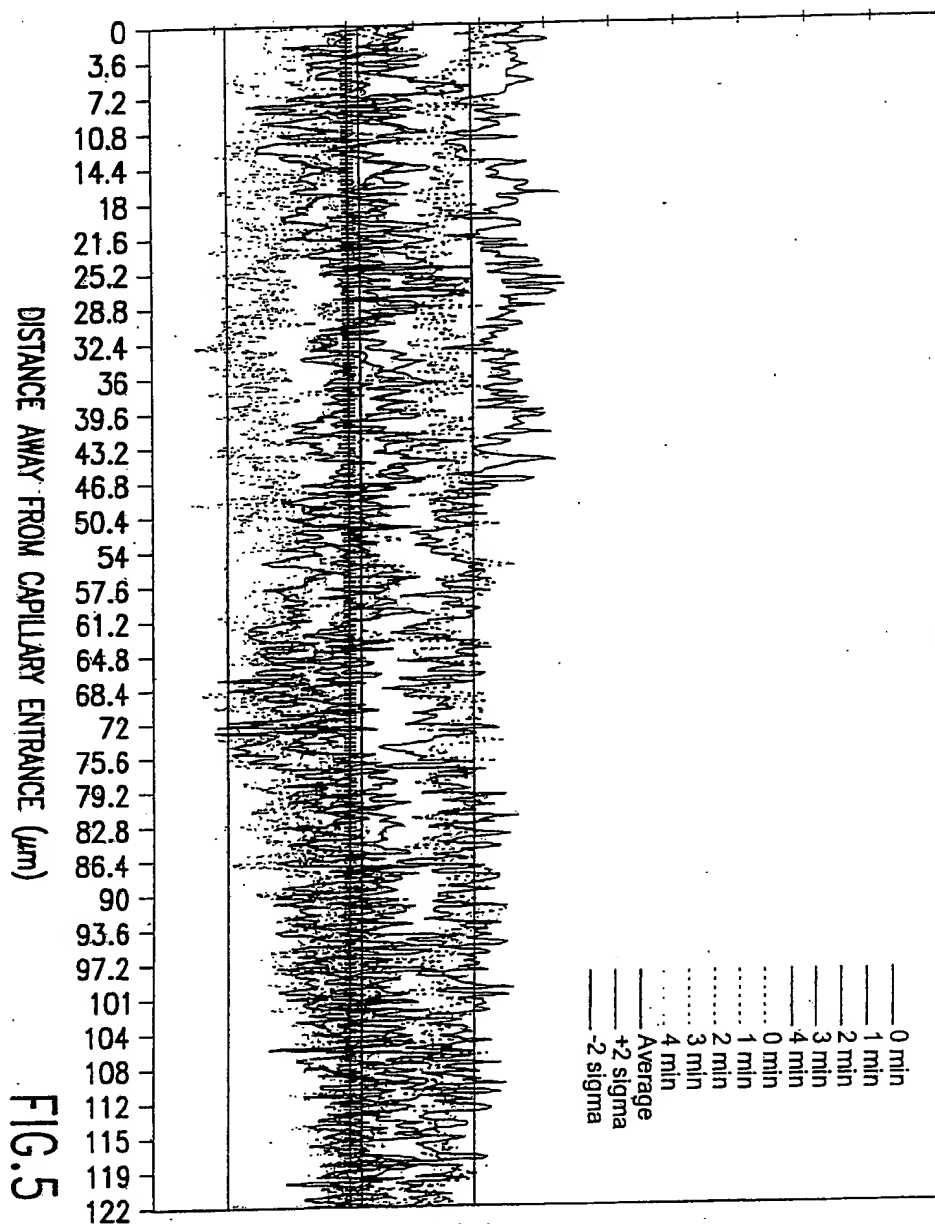

Best Available Copy



Replacement Sheets

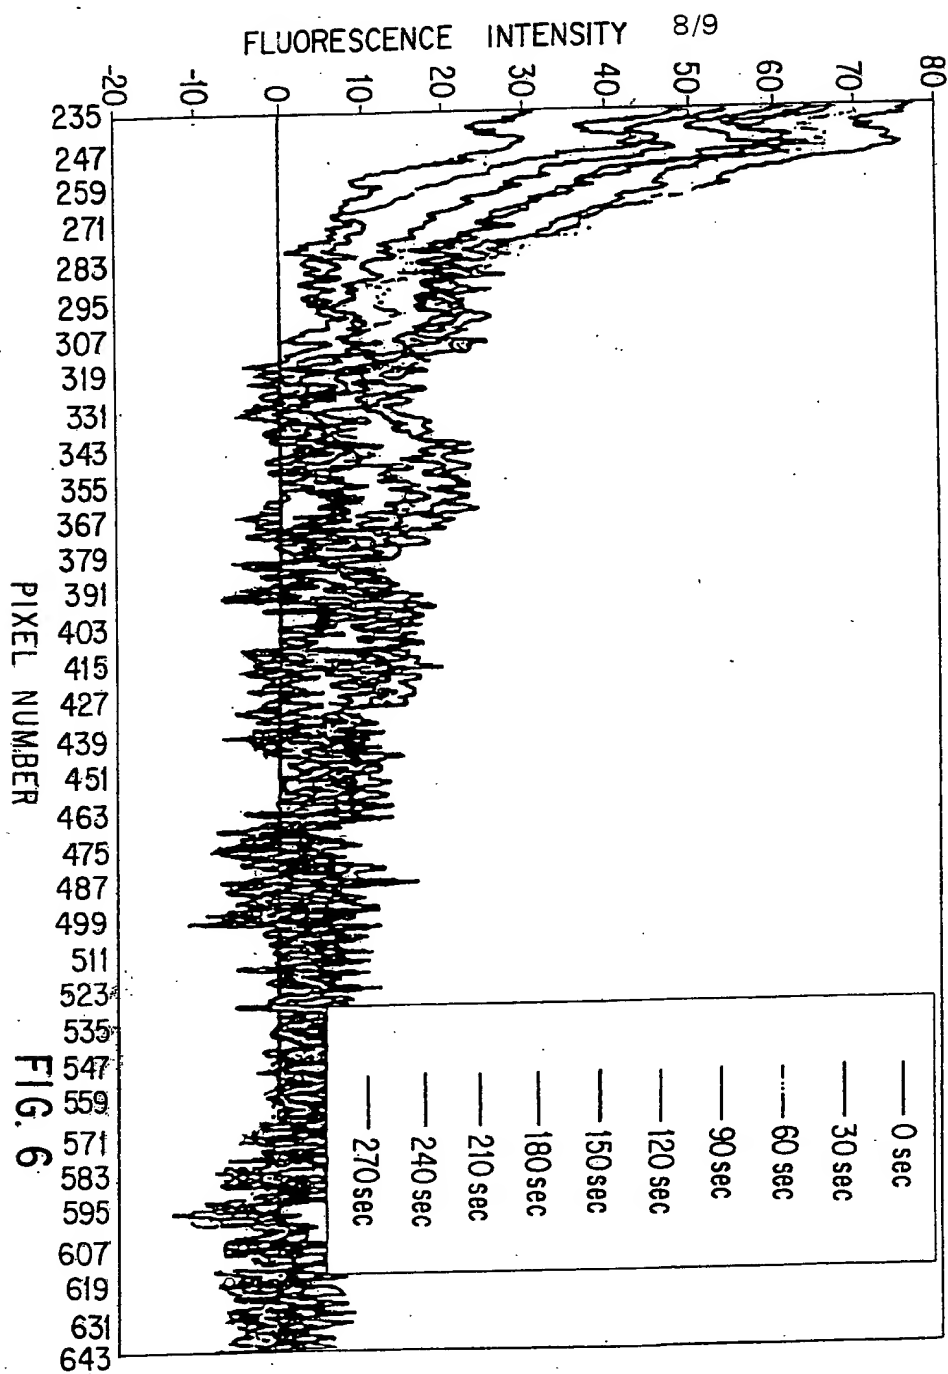

Best Available Copy



Replacement Sheets

9/9

LATEX SPHERES AT INITIAL CONCENTRATION $[C_0]$

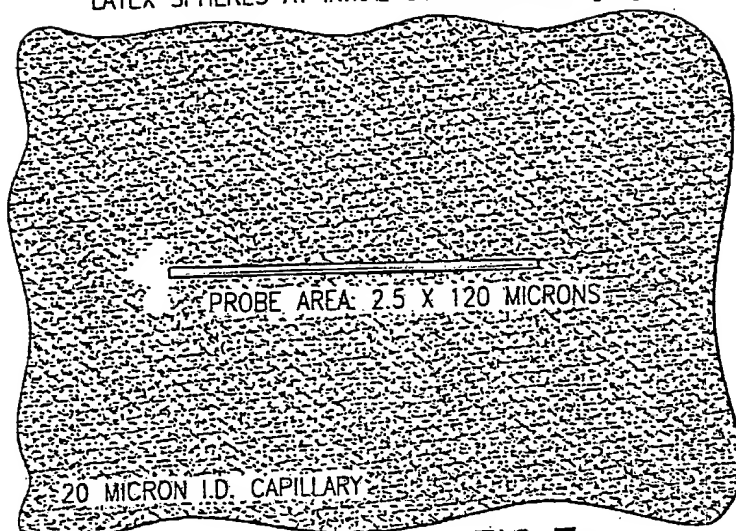


FIG.7a

4 MINUTE FOCUS, -14 kV, 30.5 mm Hg, 40.5 cm TUBE

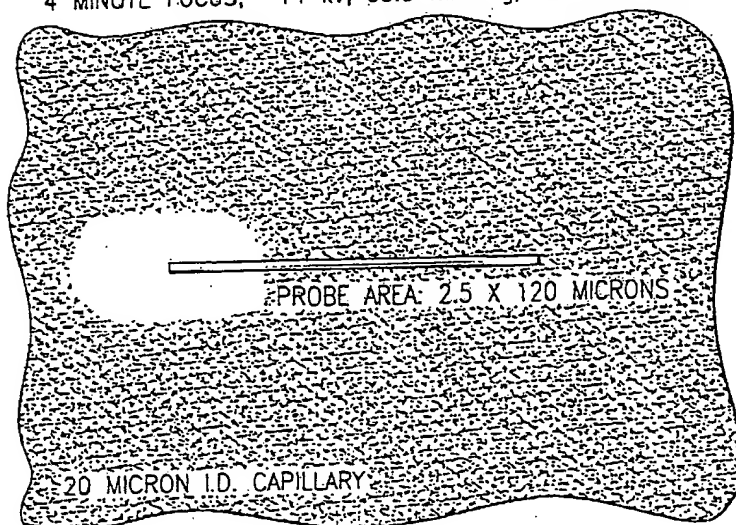


FIG.7b